



ISSN: 0975-833X

Available online at <http://www.journalcra.com>

INTERNATIONAL JOURNAL
OF CURRENT RESEARCH

International Journal of Current Research
Vol. 12, Issue, 04, pp.11163-11166, April, 2020

DOI: <https://doi.org/10.24941/ijcr.38422.04.2020>

RESEARCH ARTICLE

PREPARATION OF CHLORIDE SELECTIVE MEMBRANE ELECTRODE

*Şükrü Kalaycı

Gazi Üniversitesi Kimya Bölümü, Ankara, Türkiye

ARTICLE INFO

Article History:

Received 28th January, 2020

Received in revised form

05th February, 2020

Accepted 28th March, 2020

Published online 30th April, 2020

Key Words:

Chloride Electrode; Determination;
Membrane Electrode; Chloride, Spring
Water.

Copyright © 2020, Şükrü Kalaycı. This is an open access article distributed under the Creative Commons Attribution License, which permits unrestricted use, distribution, and reproduction in any medium, provided the original work is properly cited.

Citation: Şükrü Kalaycı. 2020. "Preparation of chloride selective membrane electrode", *International Journal of Current Research*, 12, (4), 11163-11166.

ABSTRACT

In this study, the novel membrane chloride-selective electrode consisting of 30% of tridodesylmethylammoniumchloride (TDMC) as the active material, 50% of PVC as the membrane matrix and 20% of dibutylphthalate (DBF) as the plasticizer was developed. In this electrode, the potential change occurs from 10^{-5} to 10^{-1} M chloride ion and the slope of linear portion corresponds to $55,0 \pm 2,0$ mV per decade change of chloride concentration. Furthermore, the interference effects of some ions, such as F^- , I^- , NO_3^- , SO_4^{2-} , Na^+ , K^+ , Cu^{2+} and Fe^{3+} were not observed. The response time and lifetime of electrode was 60 s and 6 months, respectively. It has been observed that pH did not affect the sensitivity of the electrode. This electrode has been used for the direct determination of $32,0 \pm 0,5$ mg/L chloride in the spring water.

INTRODUCTION

In the literature, there were several liquid and polymer membrane-based ion-selective electrodes (ISEs) used for the determination of chloride (Oka, 1981; Hartman, 1978; Willis, 1983; Hitachi, 1982; Coetzee, 1968; Coetzee, 1969). The active components in these electrodes were the quaternary ammonium salts. The innate Hofmeister-type response of such sensors to lipophilic anions, such as salicylate, can lead to significant positive errors for determination of chloride in the blood samples obtained from patients with ingested Aspirin (Lewandowski, 1989). Additionally, the positive interferences of bromide and added heparin can be also observed (Park, 1991). The researchers developed a method for the fast preparation of chloride selective electrodes (Ag/AgCl electrodes) by dipping silver wire into the sodium hypochlorite solution (Jiang, 2015). They were prepared by different immersion time. Some properties of them, such as Nernst response, response time and long-term stability, were tested in the simulated concrete pore solutions (SCPS) (Duffó, 2009; Climent, 1996). In principle, the determination of chloride is important in many different fields, such as clinical diagnosis (Jiang, 198; Huber, 1998) environmental monitoring (Huber, 2000; Martin, 1997) and various industrial applications (Badr, 1999; Ratjen, 2003).

In general, the chloride ions associated with ions Na^+ , K^+ , Mg^{2+} are present in the sea water and sediments of the Earth's crust in large quantities. Moreover, they are widely distributed to the nature as salts, such as NaCl, KCl, and $CaCl_2$ (Department of National Health and Welfare, 1978). We have developed a new chloride selective electrode because of the fact that the determination of chloride in the spring water samples is essential (Somer, 2001). The aim of this work was to prepare a selective electrode for chloride using ion exchanger as the active material. For this, the solid membrane electrodes were prepared using tridodesylmethylammoniumchloride (TDMACl), PVC and dibutylphthalate (DBF) in different compositions which were used as ion exchanger active material, inert matrix and plasticizer, respectively. Furthermore, their optimum working conditions were also investigated in detail and the interference studies were also performed. Then, the chloride ion in the spring water was determined by this prepared electrode.

Experimental

Apparatus and reagents: The potential was measured with JENWAY 3030 Ion Analyser. While a double junction Ag/AgCl electrode, 924036, was used as the outer reference electrode, as the inner reference electrode, the home-made Ag/AgCl electrode was prepared; it was immersed into a 0.1 M NaCl and 0.1 M KI solution. For the pH measurements, the ion analyser with 924003 combined with pH electrode was used. All measurements were performed with a 30 mL glass cell prepared for this purpose. A magnetic stirrer was used throughout the experiments.

*Corresponding author: Şükrü Kalaycı,
Gazi Üniversitesi Kimya Bölümü, Ankara, Türkiye.

All reagents (NaCl, KBr, NaF, KI, Fe₂(SO₄)₃, CuCl₂, AgNO₃) were of at least analytical reagent grade (Merck). Triply distilled water purification system was used for the preparation of all solutions.

Preparation of electrode: 100–250 mg of PVC dissolved in 3 mL tetrahydrofuran (THF), 90 mg of ion exchanger dissolved in 1 mL THF and 0.2 mL of DBF were mixed in a 30 mL beaker with a diameter of 4.2 cm and then the mixture was stirred by a magnetic stirrer. The solvent was then allowed to evaporate at ambient atmosphere for about 24 h. The membrane formed as a film in the bottom of the beaker was taken out carefully using Teflon forceps. Then, the film membrane was cemented to the flat end of a PVC tube (1 cm diameter) with an adhesive of PVC dissolved in THF. One day later, the excess membrane was cut and the tube was filled with 0.1 M NaCl and 0.1 M KI solution, respectively. A homemade Ag/AgCl electrode was then immersed as the inner reference electrode. For conditioning of the electrode, it should stay in 10⁻⁴ M NaCl solution for about 2 days (19).

RESULT AND DISCUSSION

Calibration curves of the electrode: The potentiometric responses of the prepared electrodes were investigated against chloride concentration. For this purpose, appropriate amounts of chloride ions were spiked to the cell and the corresponding potentials were recorded. For a fixed ionic strength, all measurements were made in 0.1 M NaNO₃ solution. The potential readings were plotted against pCl. The slope of the electrode was found as about 58 mV and it was not changed for more than 6 months.

Effect of membrane composition and thickness: It is known that the detection limit, selectivity and the maintenance of the electrode depend on membrane composition and thickness. For this reason, the electrodes in different membrane compositions and thickness were prepared and their potential responses were measured in the range from 10⁻⁶ to 10⁻¹ M chloride concentration for each 10 times of concentration change. By the time membrane mixtures in different weight quantities were used in the same size of beakers, the thickness of membranes was also different. The membranes in 30% of TDMACl, 50% of PVC and 20% of DBF composition but at different masses (0.2, 0.3, 0.4 and 0.5 g) were prepared and they were used as the active materials. For each electrode, the potential responses were measured at different chloride concentrations. In the concentration range from 10⁻⁵ to 10⁻¹ M chloride, the slopes for 0.2, 0.3, 0.4 and 0.5 g of electrodes were about 24, 21, 58 and 31 mV, respectively (Fig. 1). It is known that the membrane thickness also plays an important role for the response of the electrodes. While the response time was short with thin membranes, its mechanical strength became less. Finally, it was found that the electrode with a total mass of 0.4 g had both the highest slope and good mechanical strength. Furthermore, to investigate the effect of composition, the electrodes in 0.4 g weight were prepared in different active material ratios, changing from 10 to 30% of TDMACl. The measured slopes of electrodes in different compositions were summarized in Table 1. As seen, because the electrode with 30% of TDMACl had the highest slope (about 58 mV), this electrode was used throughout the whole study.

The response time of electrode: The response time of the electrode was measured for different chloride concentrations because it depends strongly on the concentration change.

Table 1. Effect of membrane composition on the response time of electrode (0.4 g) in 0.1 M NaNO₃

(F ⁻) (M)	E (mV)	20%TDMACl, 60%PVC, 20%DBF	30%TDMACl, 50%PVC, 20%DBF
1x10 ⁻⁵	192	180	152
1x10 ⁻⁴	174	155	100
1x10 ⁻³	150	125	40
1x10 ⁻²	131	90	-20
1x10 ⁻¹	105	50	-80
1x10 ⁻⁵ to 1x10 ⁻¹ M Slope	21.8	32.5	58.0

Table 2. Selectivity coefficients ($K_{A,B}^{pot}$) for the chloride selective electrode in mixed solutions (in the presence of 1x10⁻⁵ M Cl⁻)

Ions	$K_{A,B}^{pot}$
Cl ⁻	2x10 ⁻³
NO ₃ ⁻	6x10 ⁻⁴
SO ₄ ⁻²	7x10 ⁻⁶
PO ₄ ⁻³	3x10 ⁻⁴
K ⁺	2x10 ⁻³
Na ⁺	1x10 ⁻³
Ag ⁺	1x10 ⁻⁵
Ca ⁺²	2x10 ⁻⁶
Cu ⁺²	3x10 ⁻⁶
Mg ⁺²	3x10 ⁻⁶

Table 3. Chloride analysis in tea and comparison of results with commercial electrodes

Ion	Developed electrode	Commercial (Orion) electrode	$t_{\text{experimental}}/t_{\text{critical}}=2,53$
(Cl ⁻) (mg/L)	32 ± 0.5	33 ± 0.6	0.42

95% Cl and N=5

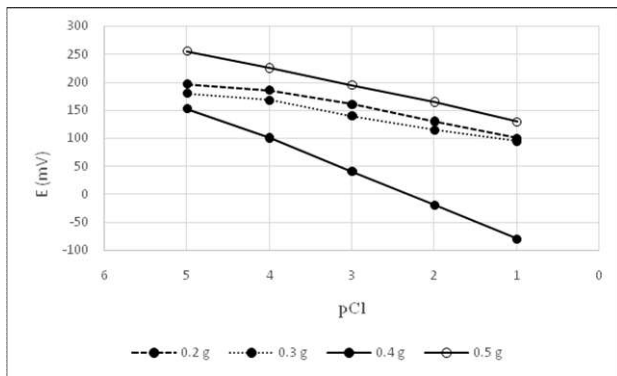


Fig. 1. Effect of membrane thickness on calibration curves (30% TDMACl, 50% PVC and 20 % DBF).

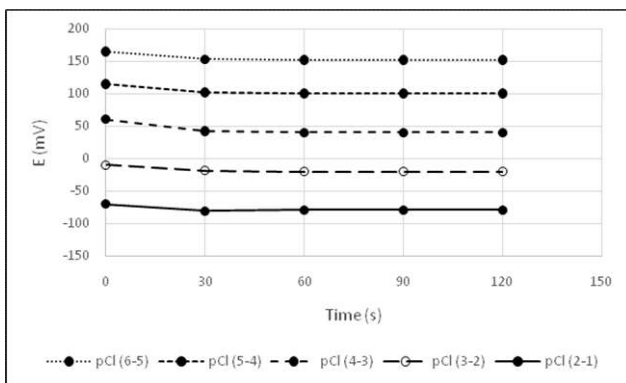


Fig. 2. The dependence of response time on the change of concentrations

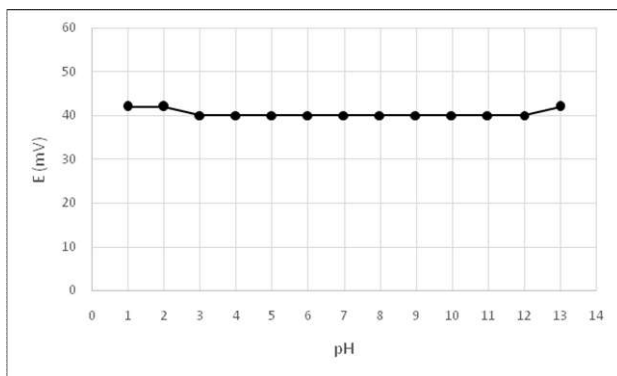


Fig. 3. Variation of the chloride electrode potential at 1.0×10^{-3} M concentration with pH

For this purpose, the potential values based on time were recorded at different chloride concentrations. The response time of the electrode was found as 1 minute (Fig. 2).

Effect of Ph: The pH effect on the potential readings at 10^{-3} M chloride concentration was investigated in detail. For this purpose, the 10^{-3} M chloride solution was prepared and the pH of this solution was adjusted to certain values by the addition of both HCl and NaOH using a pH meter. For chloride concentration, the measured potentials at each pH values were plotted against pH. The potential readings remained unchanged within the pH range of 2–12 at 10^{-3} M chloride concentrations of chloride (Fig. 3).

Interference studies: The possible interference effects of some anions (F^- , Br^- , I^- , SO_4^{2-}) and cations (Na^+ , K^+ , Cu^{2+} , Fe^{3+})

were investigated. For this, selectivity coefficients mixed solution method was preferred as it usually corresponds more closely to the situation in the samples. In this method, solutions were prepared with a constant activity of the main ion (chloride) while varying activity of interfering ion. For this purpose, the interfering ion was added to 10^{-3} M chloride solution (in 0.1 M $NaNO_3$) so that its concentration was 10^{-2} to 10^{-3} M and after each addition, the change of potential was measured. Based on the experimental results, no interference effect was observed for F^- , Br^- , I^- , SO_4^{2-} and for Cu^{2+} , Fe^{3+} .

The selectivity coefficients for the interfering ions were also calculated by using the mixed solution method (20).

$$K_{A,B}^{pot} x a_B^{n_A/n_B} = a_A \{ \text{antilog}((E_1 - E_2)/S) \} - a_A \quad (1)$$

where $S = 2.303RT/n_A$ (the slope of chloride electrode), a_A is the activity of the primary ion, a_B is the activity of the interfering ion, E_1 is the potential measured when only A is present, E_2 is the potential responsive to the primary ion in the presence of interfering ion. $K_{A,B}^{pot}$ the selectivity coefficient and n_A , n_B are the charges of A and B, respectively. For the determination of the selectivity constant, the $a_B^{n_A/n_B}$ values were plotted against the right hand side of Eq. (1) and the slope was equal to the selectivity coefficient of the interfering ions. The selectivity coefficients obtained for some anions and cations were given in Table 2.

Determination of chloride in spring water: For this purpose, 500 mL of spring water sample was taken for the determination of chloride ion. The potential measurements in the sample including 0.1 M $NaNO_3$ were made using both the commercial electrode and the electrode prepared in this study. For the determination of chloride ion in the sample, different calibration graphs were drawn for both electrodes. From both calibration graphs, while the chloride concentration was determined as 33.0 ± 0.6 mg/L with commercial (Orion) electrode, it was determined as 32.0 ± 0.5 mg/L with the newly prepared electrode. The results were given for both electrodes based on 95% of confidence level using five different samples. The t-test was performed to compare the means of the results obtained from both electrodes. Based on the calculations, the results of both commercial and electrode prepared in this study were similar shown in Table 3.

Conclusion

In this proposed study, the new a selective electrode was used for the determination of chloride. This electrode showed 58 mV sensitivity to chloride concentrations in the range from 10^{-5} to 10^{-1} M. As a result of the analysis, the chloride concentration in the spring water sample was found to be 32 ± 0.5 mg/L based on 95% of confidence level in five measurements.

REFERENCES

- Climent-Llorca, M.A., Viqueira-Perez, E., Lopez-Atalaya, M.M. 1996. Embeddable Ag/AgCl sensors for In-situ monitoring chloride contents in concrete (J). *Cement and Concrete Research*, 26 (8), 1157–1161.
- Coetzee, C. V., Freiser, H. 1969. Liquid-liquid membrane electrodes based on ion-association extraction systems, *Anal. Chem.* 41, 1128-1130.

- Coetzee, C. V., Freiser, H. 19868. Anion-responsive electrodes based on ion association extraction systems, *Anal. Chem.* 40, 2071-2071.
- Department of National Health and Welfare (Canada). Guidelines for Canadian drinking water quality. Supporting documentation. Ottawa, 1978.
- Duffó, G.S., Farina, S.B., Giordano, C.M. 2009. Characterization of solid embeddable Reference electrodes for corrosion monitoring in reinforced concrete structures (J). *Electrochimica Acta*, 54 (2009), 1010–1020.
- Hartman, K., Luterotti, S., Osswald, H., Oehme, M., Meyer, P., Ammann, D., Simon, W. Chloride-selective liquid-membrane electrodes based on lipophilic methyl-tri-N-alkyl- ammonium compounds and their applicability to blood serum measurements, *Microchim. Acta*, 70 (3-4) (1978), 235-246.
- Hitachi, Ltd. Jpn. TokkyoKoho No. 5,757,655, 1982.
- Huber, C., I. Klimant, C. Krause, T. Werner, T. Mayr, O.S. Wolfbeis, *Fresenius J. Anal. Chem.* 368 (2000), 196-202.
- Huber, C., T. Werner, C. Krause, I. Klimant, O.S. Wolfbeis, Energy transfer-based lifetime sensing of chloride using a luminescent transition metal complex, *Anal. Chim. Acta* 364 (1998), 143-151.
- Badr, I.H.A. M. Diaz, M.F. Hawthorne, L.G. Bachas, Mercuracarborand “Anti-Crown Ether”-Based Chloride-Sensitive Liquid/Polymeric Membrane Electrodes, *Anal. Chem.* 71 (1999), 1371-1377.
- Jiang, L., Liu, H., Wang, Y. 2015. Influence of flexural fatigue on chloride threshold value for the corrosion of steels in Ca (OH)₂ solutions (J). *Materials Chemistry and Physics*, 23–28.
- Jiang, Q. S., Mak, D., Devidas, S., Schwiebert, E.M., Bragin, Zhang, A.Y.L., Skach, W.R. W.B. Guggino, J.K. Foskett, J.F. Engelhardt, Cystic fibrosis transmembrane conductance regulator-associated ATP release is controlled by a chloride sensor, *J. Cell Biol.* 143 (1998), 645-657.
- Lewandowski, V., Sokalski, T., Hulanicki, A. 1989. Influence of aspirin on in vitro direct potentiometry of Cl⁻ in serum, *Clin. Chem.* 35, 2146-2146.
- Martin, A., Narayanaswamy, R. Studies on quenching of fluorescence of reagents in aqueous solution leading to an optical chloride-ion sensor, *Sensor and Actuator B-Chem.* 39 (1997), 330-333.
- Oka, S., Sibasaki, Y., Tahara, S. 1981. Direct potentiometric determination of chloride ion in whole blood, *Anal. Chem.* 53, 588-593.
- Park, S. B., Matuszewski, W., Meyerhoff, M.E., Liu, Y. H., Kadish, K.M. 1991. Potentiometric anion selectivities of polymer membranes doped with indium(III)-porphyrins, *Electroanalysis* 3, 909-913.
- Ratjen, F., Doring, G. 2003. Cystic fibrosis, *Lancet*, 361 (2003), 681-689.
- Somer, G. Ş. Kalaycı, G. Ekmekci, Preparation and application of iodide-mercury selective membrane electrode based on ion exchangers, *Sensors and Actuators B*, 81 (2001), 122-127.
- Srinivasan, K., Rechnitz, G.A. 1969. Selectivity studies on liquid membrane, ion selective electrodes, *Analytical Chemistry*, 41(10), 1203-1208.
- Willis, J., Young, C., Martin, R., Stearns, P., Pelosi, M., Magnanti, D. 1983. The Clinical- evaluation of bis crown ether based potassium-ion selective electrodes, *Clin. Chem.* 29, 1193-1198.
